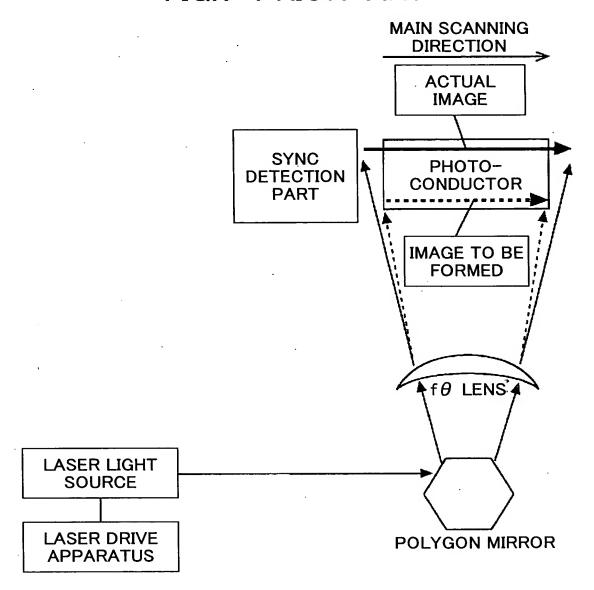
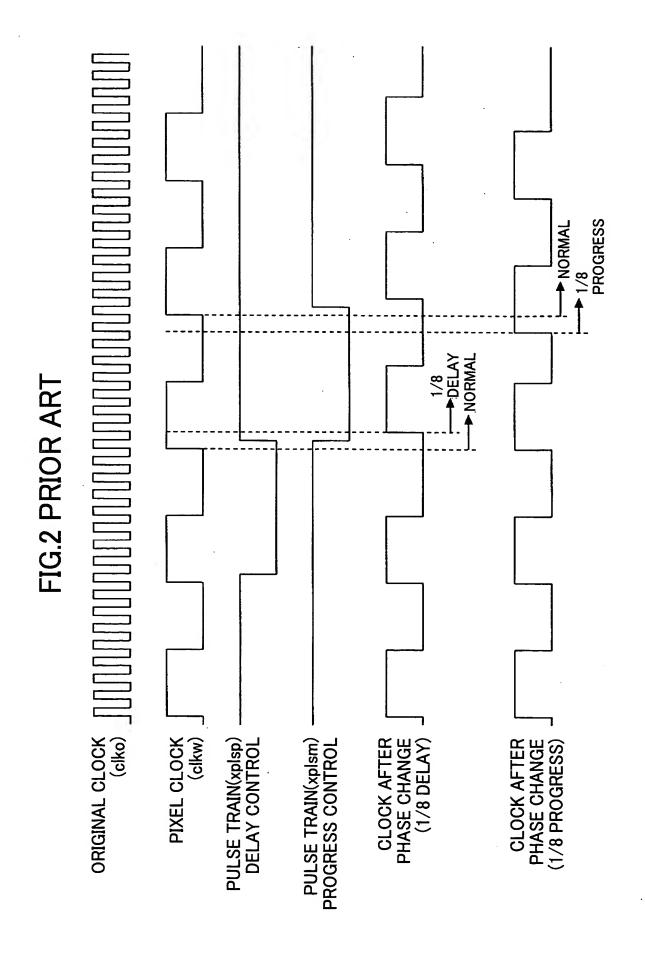
FIG.1 PRIOR ART





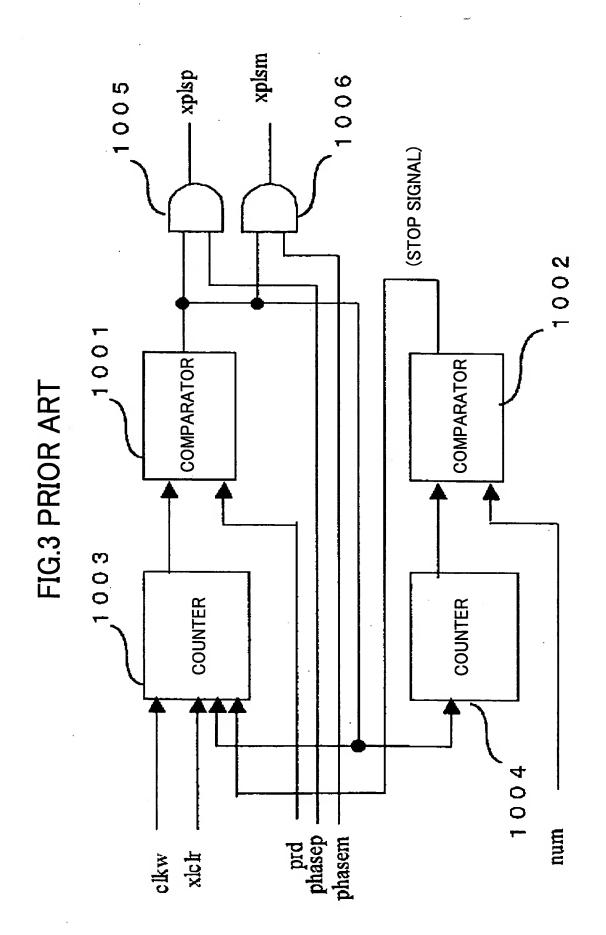
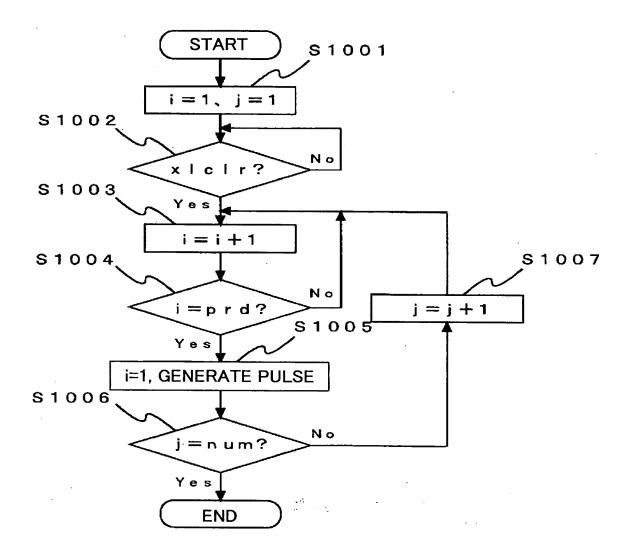
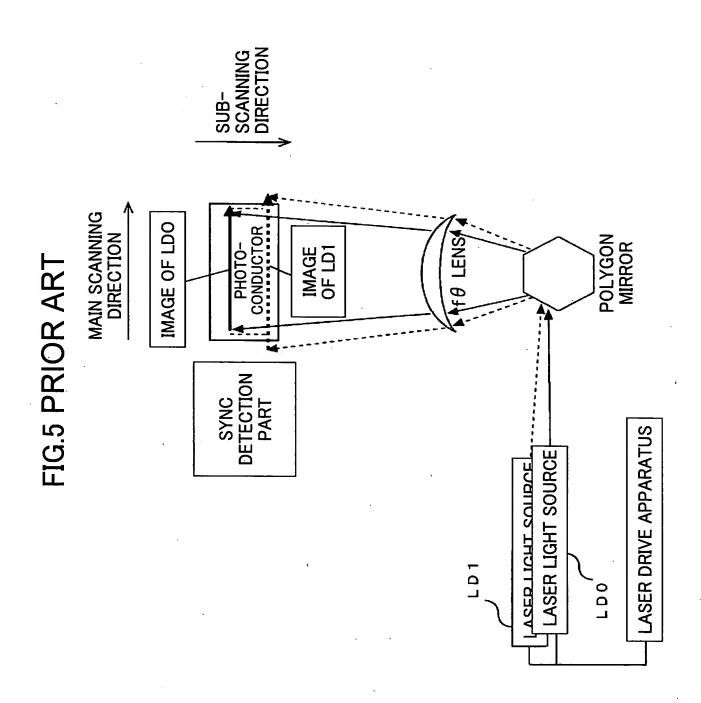


FIG.4 PRIOR ART





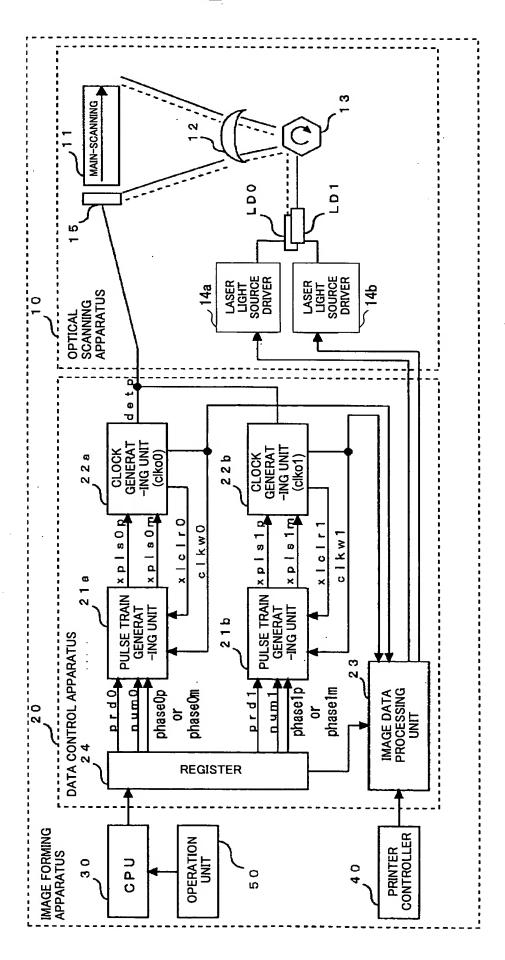


FIG 6

FIG.7A

MAIN-SCANNING



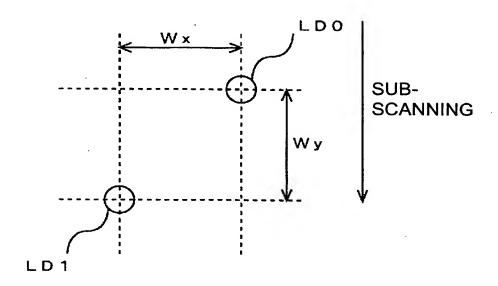


FIG.7B

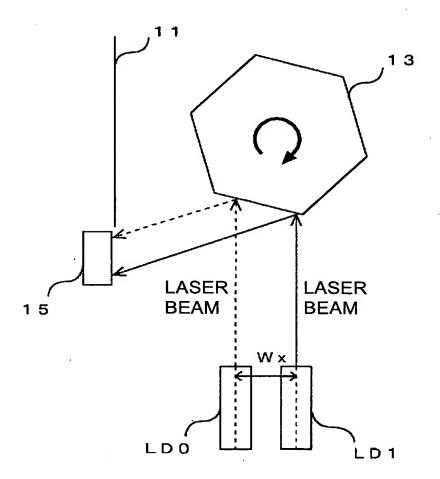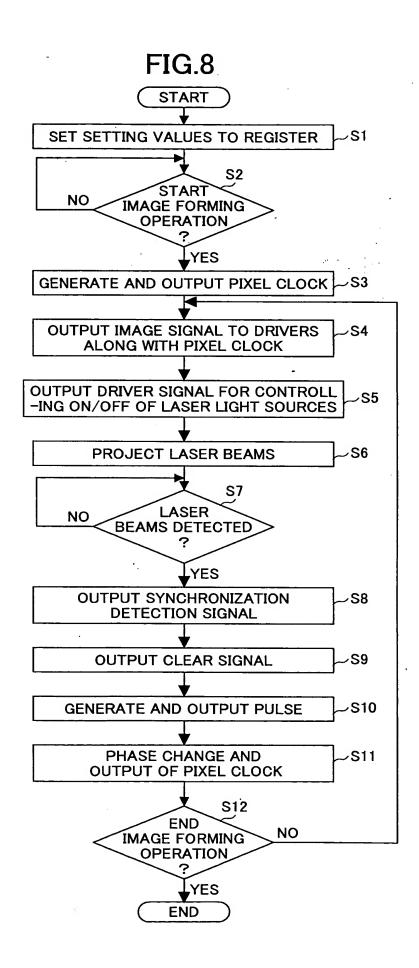

OBLON, SPIVAK, ET AL DOCKET #:249155US2 INV: Yoshiki YOSHIDA SHEET 8 OF 38



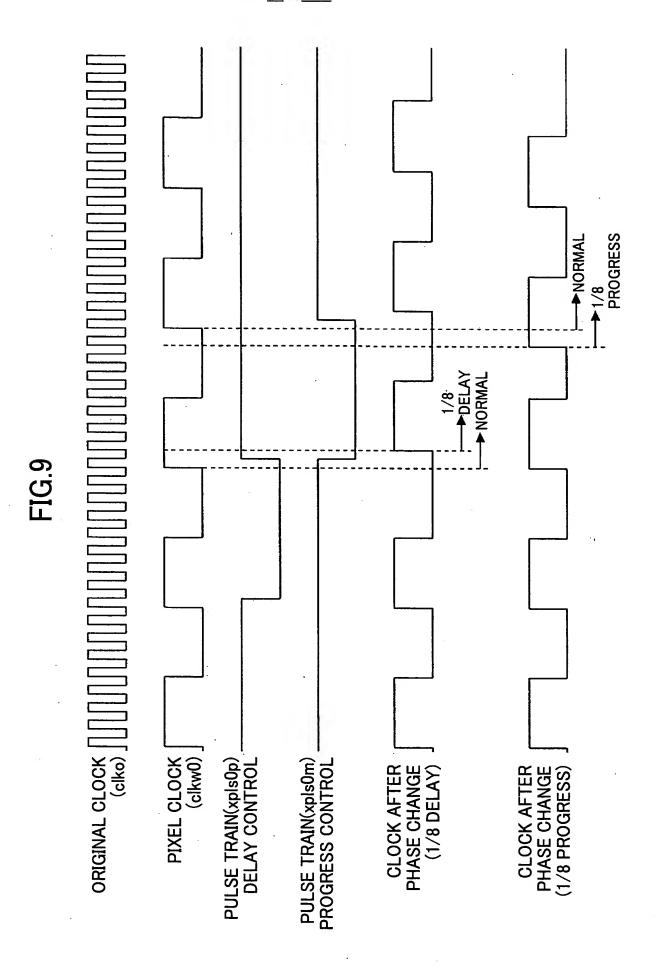


FIG.10

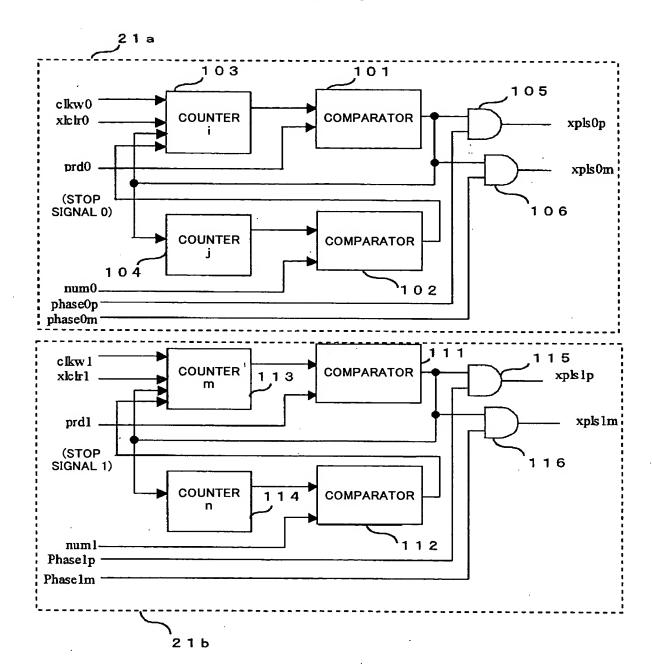
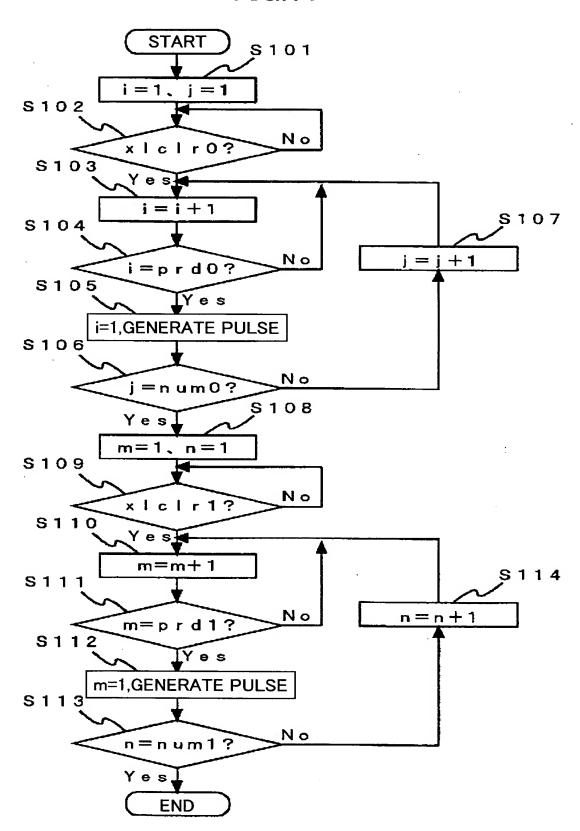


FIG.11



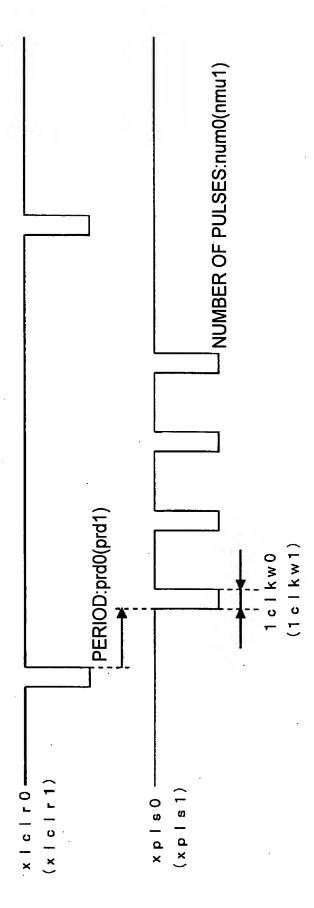


FIG.12

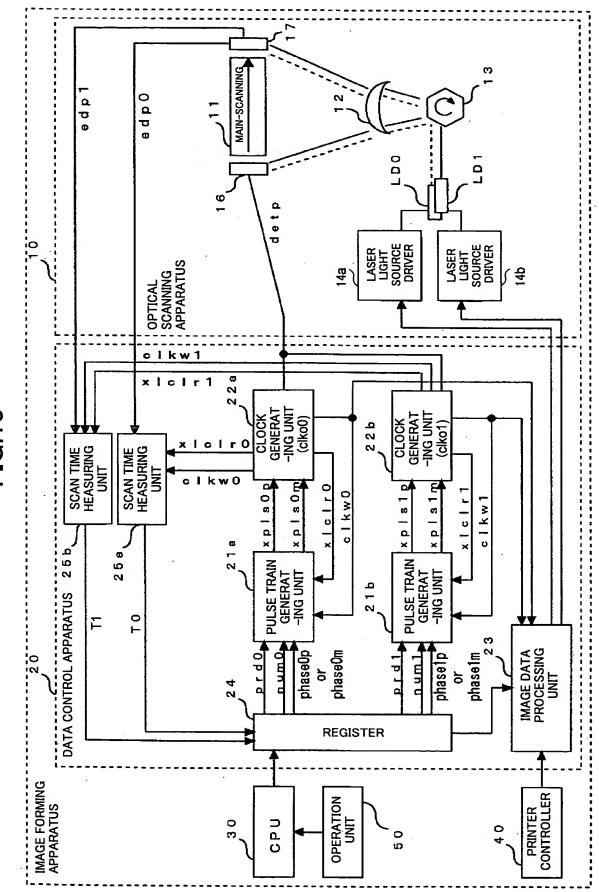


FIG.13

edp1

J×lolrJ

SCAN TIME MEASURING UNIT 25b (LD1)

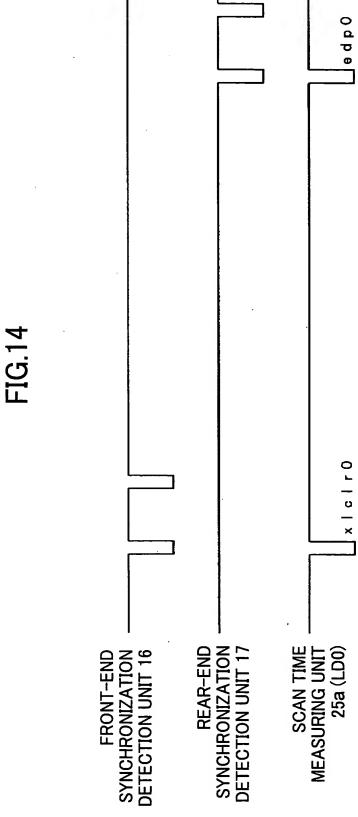


FIG.15A

MAIN-SCANNING

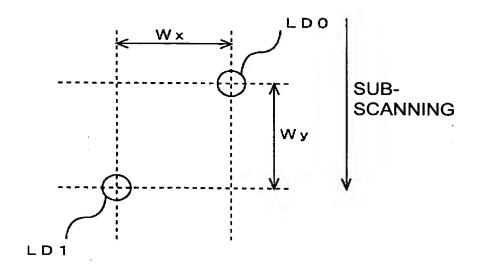
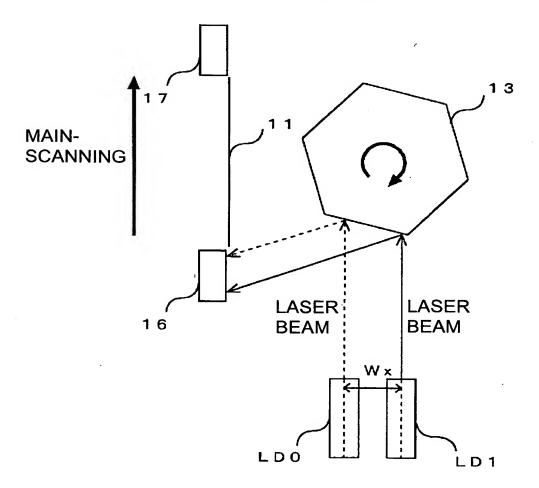


FIG.15B



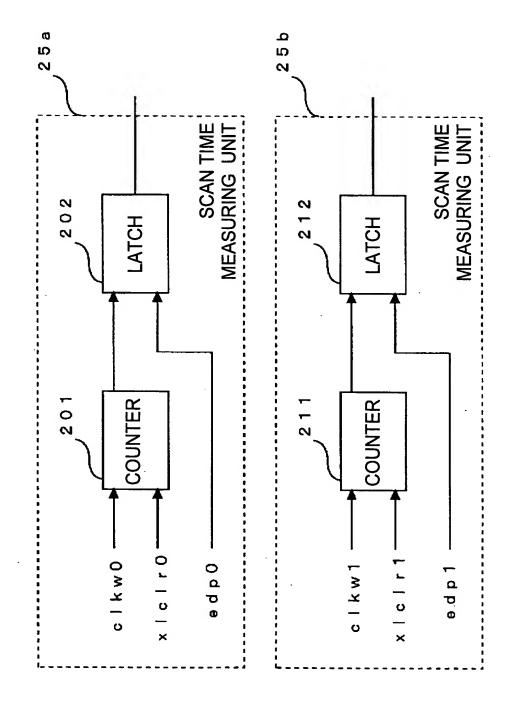
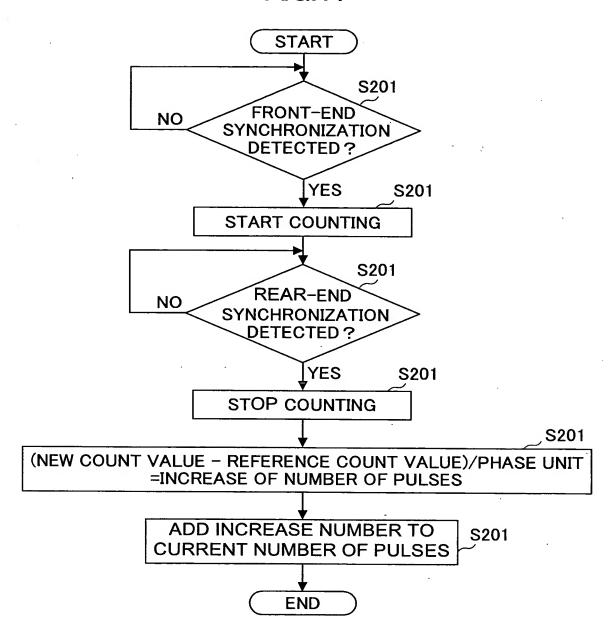
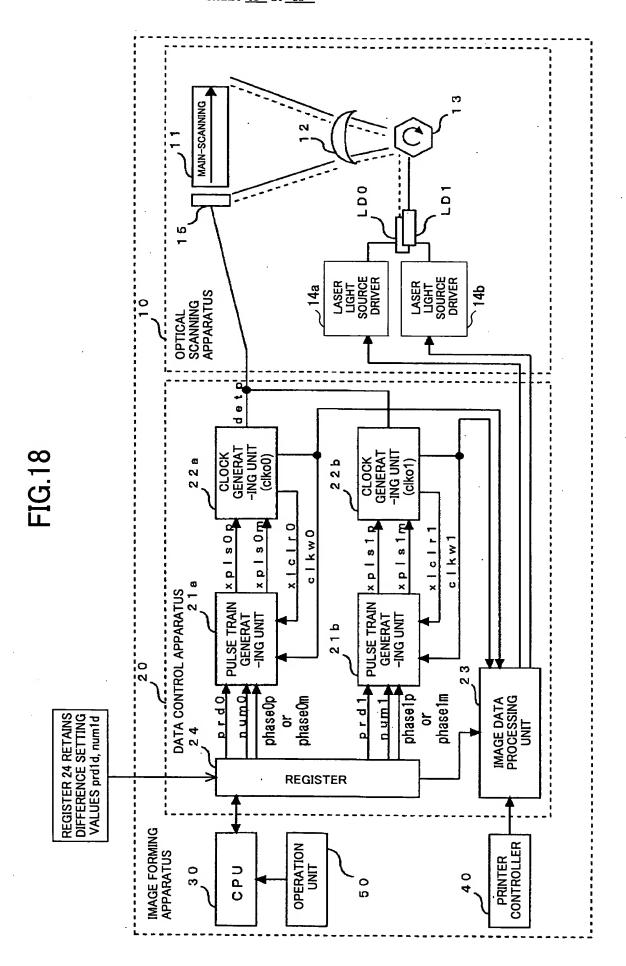


FIG.16

FIG.17





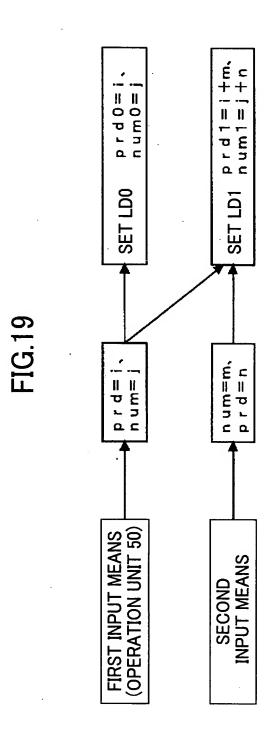
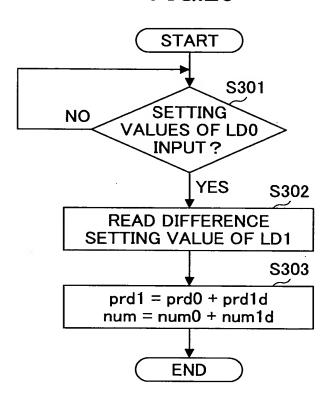


FIG.20



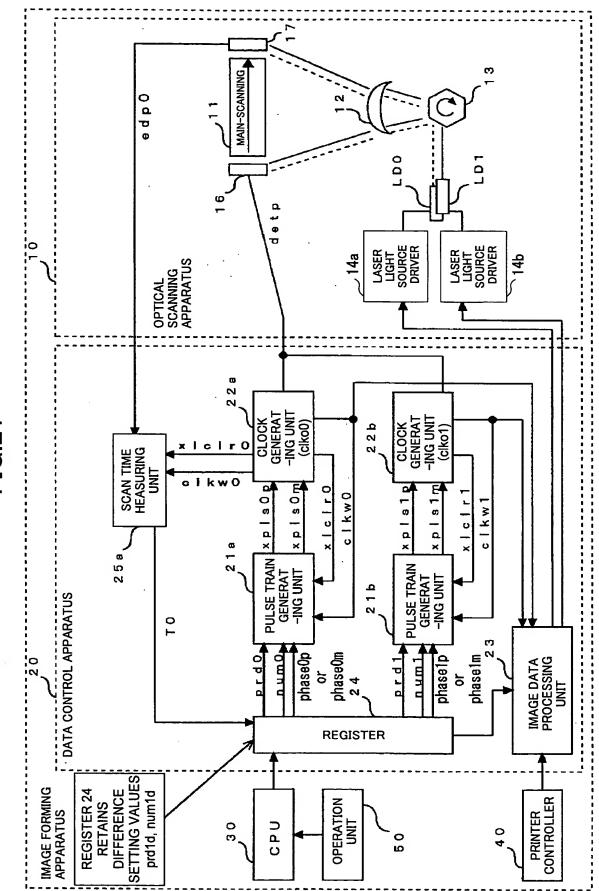
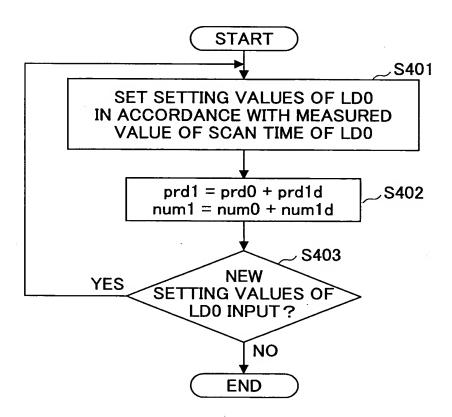


FIG.21

FIG.22



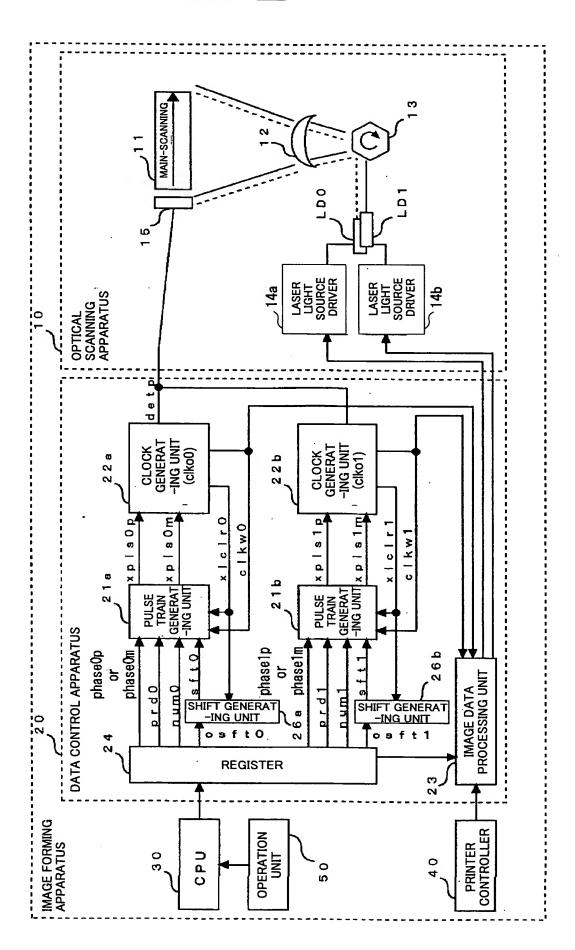


FIG.23

FIG.24



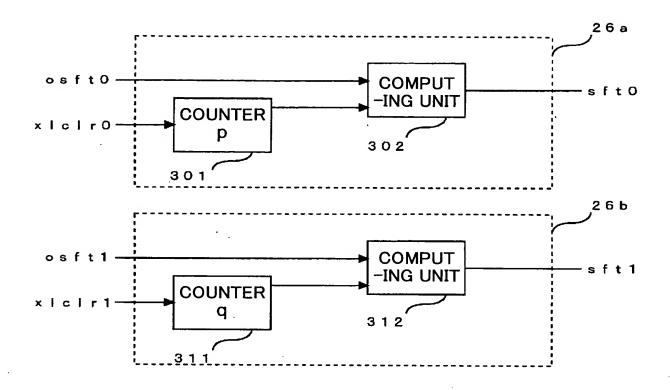



FIG.25

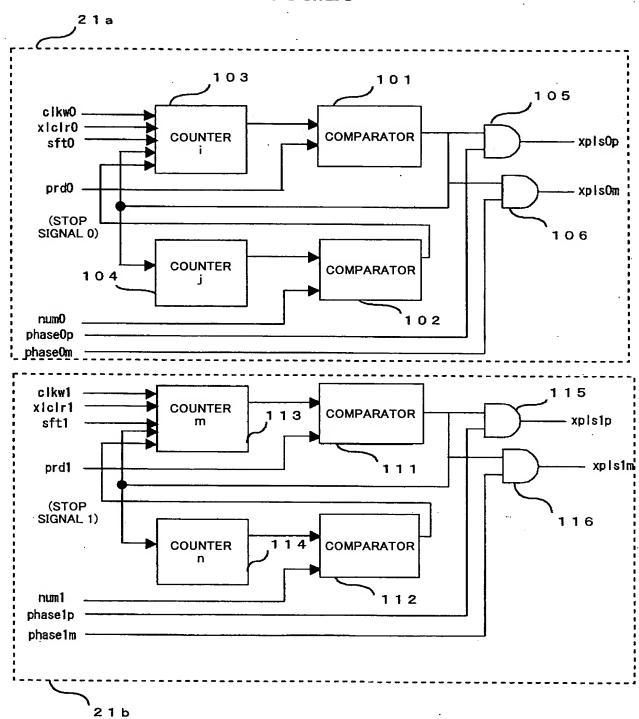

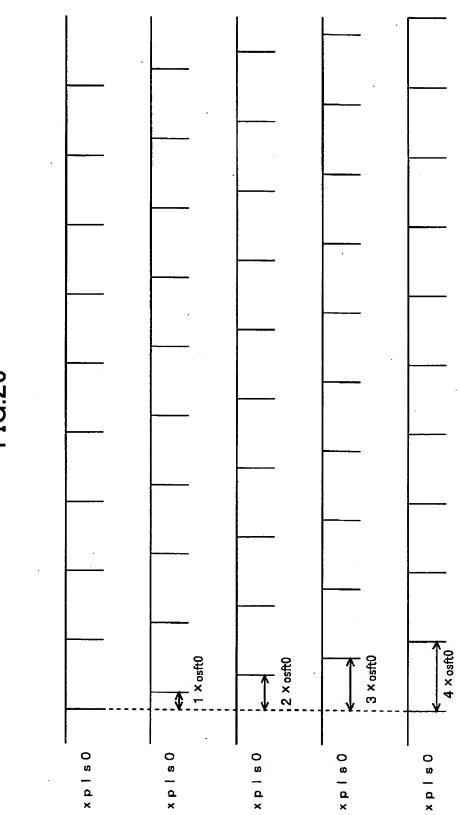

19.26

FIG.27

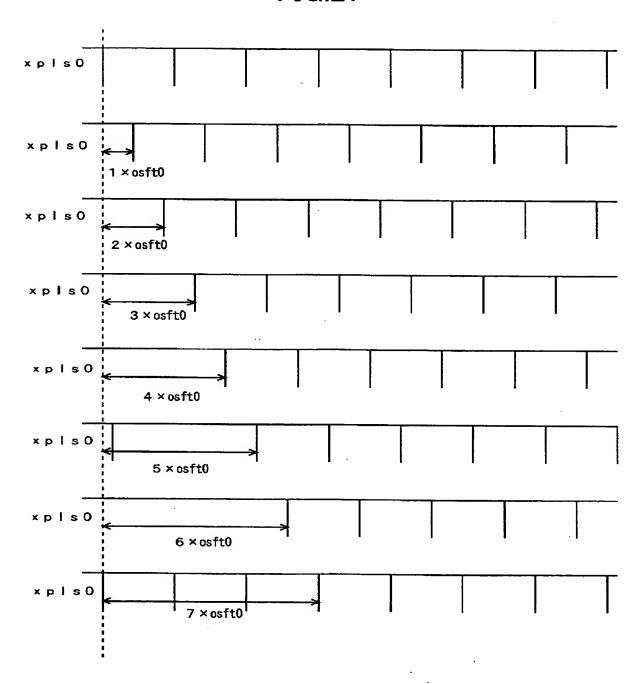

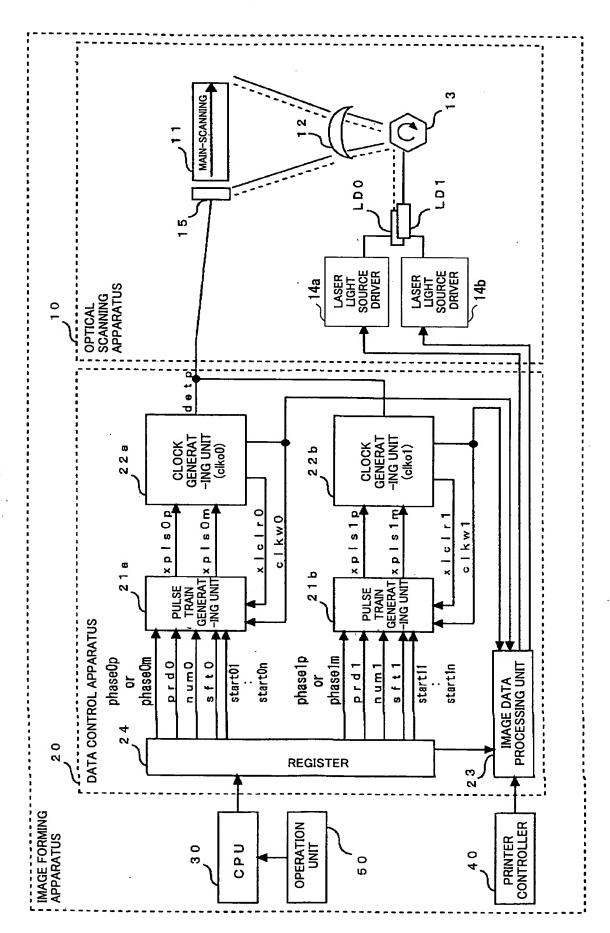
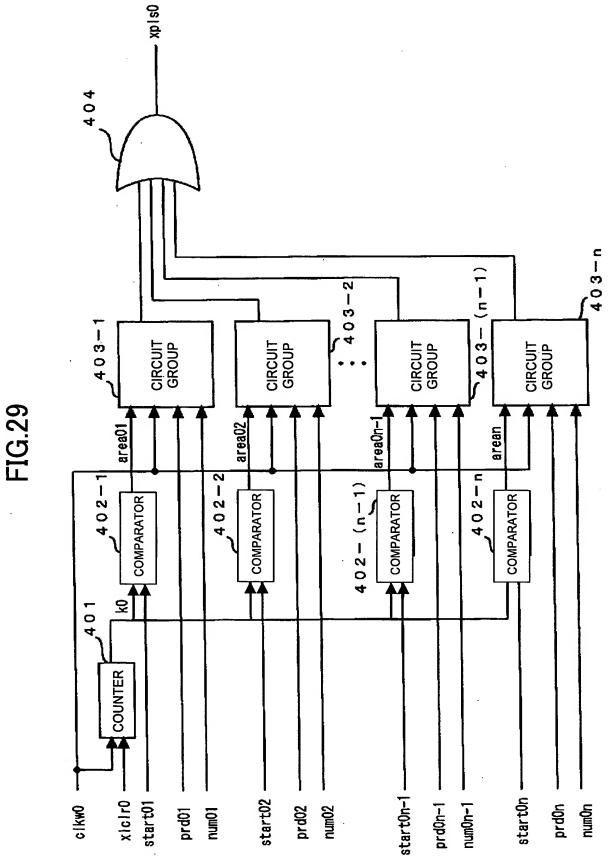


FIG.28



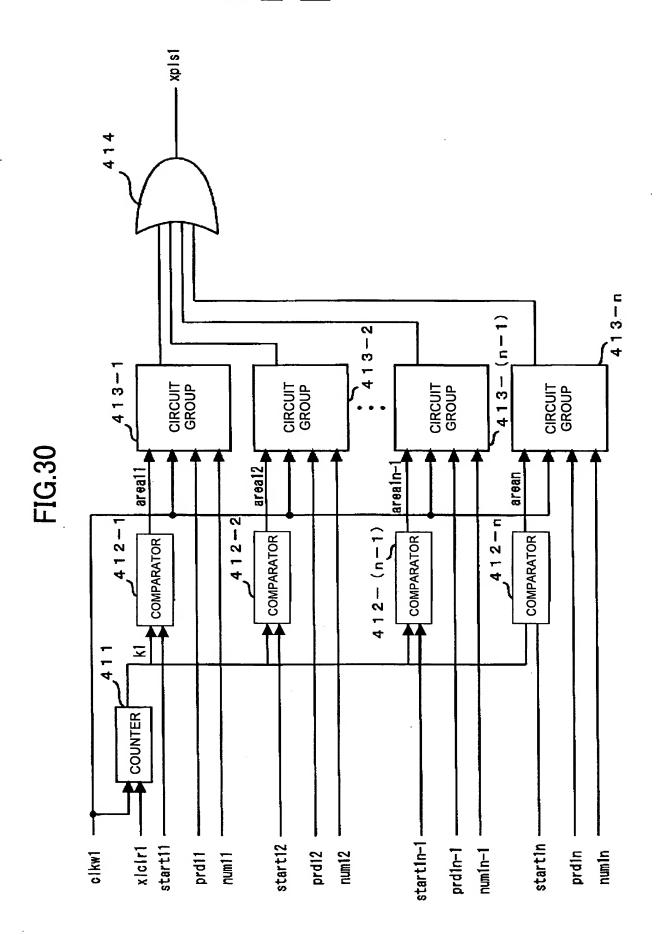
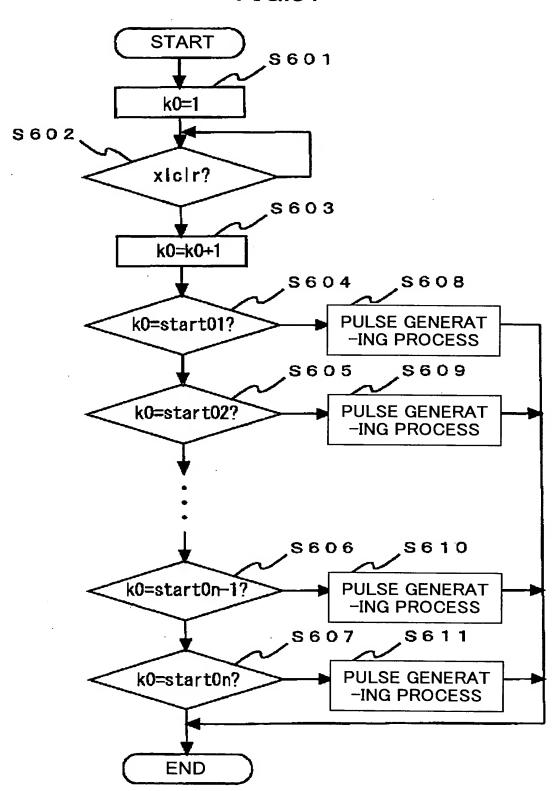
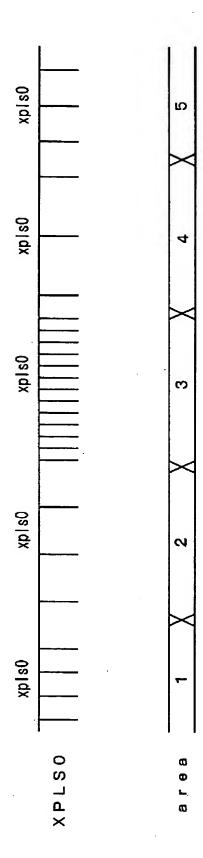


FIG.31







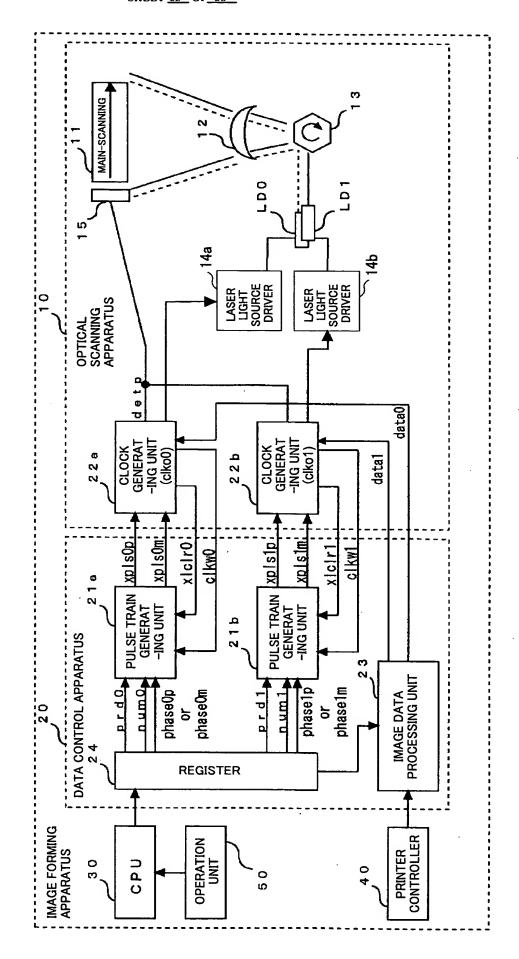
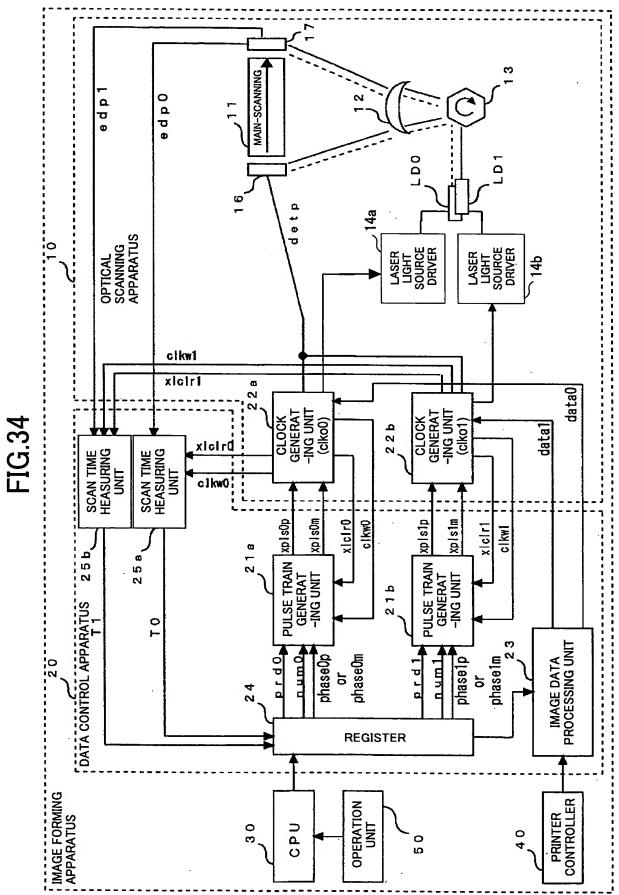


FIG.33



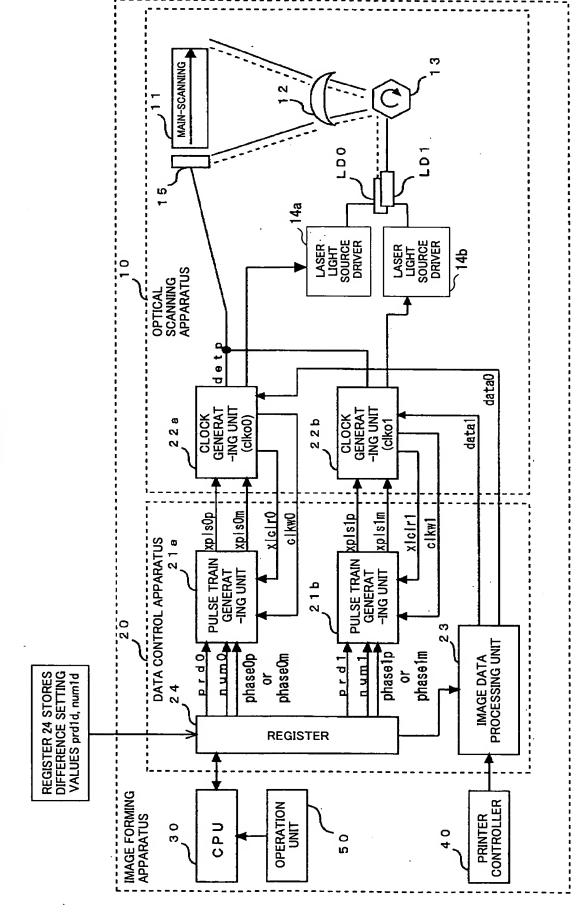


FIG.35

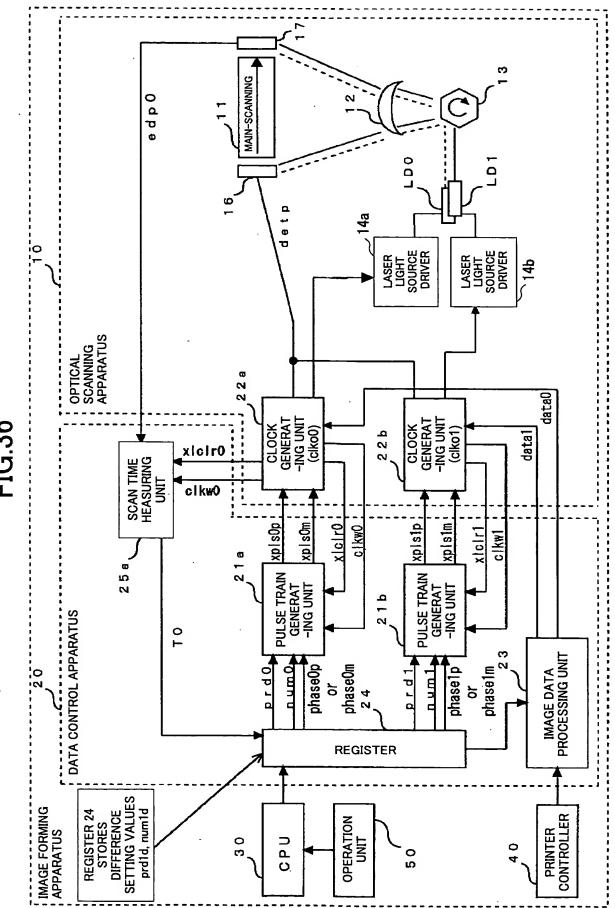


FIG.36

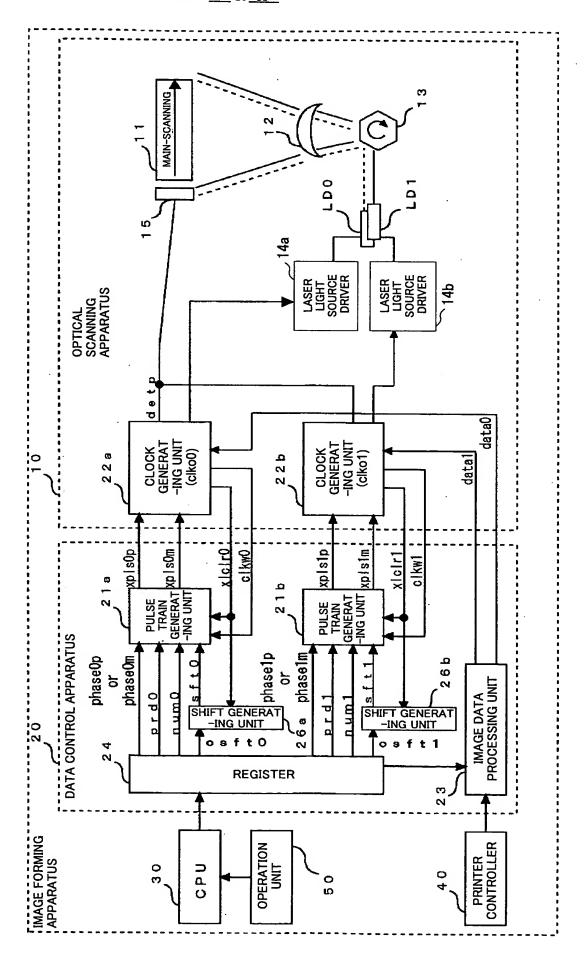


FIG.37

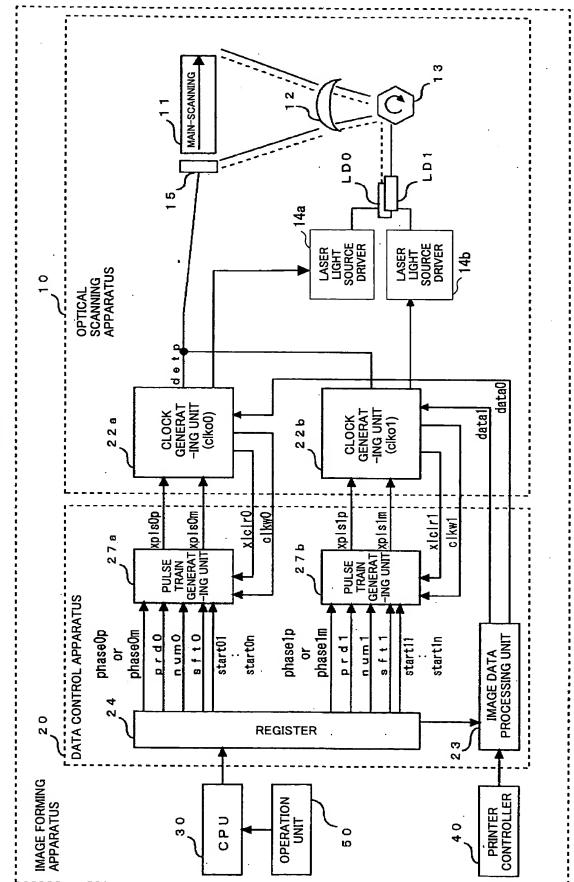


FIG.38

١,